


SDP31

Quick start guide for differential pressure evaluation kit

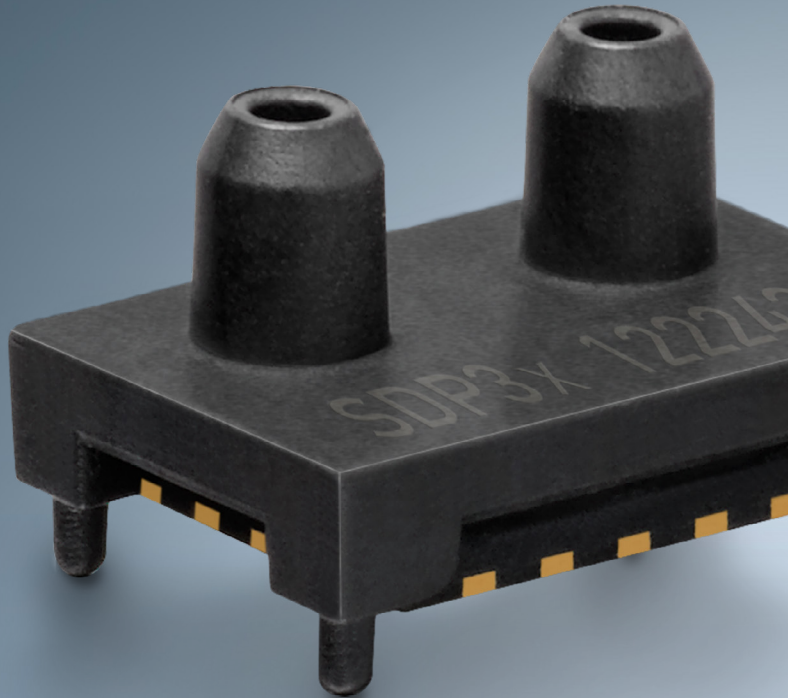

SENSIRION

01


Set-up

- Install the last version of the Sensirion ControlCenter Software from the website.
- Connect the Sensor-PCB to the flow channel.
- Connect the sensor to a PC via the SEK-SensorBridge. The cable to connect the sensor with the SEK-SensorBridge is included in the evaluation kit.

02

Getting started with the Sensirion ControlCenter Software

- Run the ControlCenter Software.
- The sensor will be identified by the software automatically.
- ① Select Config  to adjust sampling rates, temperature compensation mode and displayed units.
- ② Select Plot Settings  to adjust the graph configurations.
- Press Start to run a measurement.

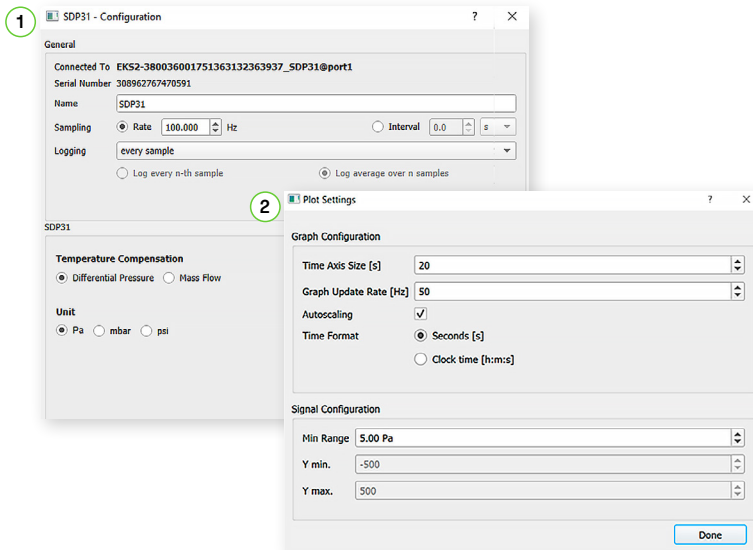

Please find all information about our differential pressure evaluation kits, including the required software, on our website: www.sensirion.com/ekdp



Thank you for your interest
in our differential pressure sensors.

Sensirion AG

Laubisrütistrasse 50 · 8712 Stäfa · Switzerland · phone +41 44 306 40 00 · info@sensirion.com
www.sensirion.com